

**INITIAL EVALUATION OF PROFILES OF TEMPERATURE, WATER VAPOR,
AND CLOUD LIQUID WATER FROM A NEW MICROWAVE PROFILING
RADIOMETER**

by

James C. Liljegren* and Barry M. Lesht
Environmental Research Division
Argonne National Laboratory
Argonne, IL 60439

Seiji Kato
Hampton University
Center for Atmospheric Science
Mail Stop 420, Hampton, VA 23681-0001

Eugene E. Clothiaux
The Pennsylvania State University
Department of Meteorology
University Park, PA 16802

for submission to

11th Atmospheric Radiation Measurement (ARM) Program Science Team Meeting,
19-23 March 2001, Atlanta, Georgia.

*Work at Argonne National Laboratory was supported by the U.S. Department of Energy, Office of Science, Office of Biological and Environmental Research, Environmental Sciences Division, under contract W-31-109-Eng-38.

The submitted manuscript has been created by the University of Chicago as operator of Argonne National Laboratory under Contract No. W-31-109-ENG-38 with the U.S. Department of Energy. The U.S. government retains for itself, and others acting on its behalf, a paid-up, nonexclusive, irrevocable worldwide license in said article to reproduce, prepare derivative works, distribute copies to the public, and perform publicly and display publicly, by or on behalf of the government.

Evaluation of Profiles of Temperature, Water Vapor and Cloud Liquid Water from a New Microwave Radiometer

James C. Liljegren¹, Barry M. Lesht¹, Seiji Kato², and Eugene E. Clothiaux³

(1) Environmental Research Division, Argonne National Laboratory, Argonne, IL

(2) Center for Atmospheric Science, Hampton University, Hampton, VA

(3) Department of Meteorology, Pennsylvania State University, University Park, PA

Corresponding author: James C. Liljegren (liljegren@anl.gov)

Introduction

The ARM Program launches approximately 2600 radiosondes each year from its Southern Great Plains (SGP) facilities in Oklahoma and Kansas, USA, to acquire vertical profiles of temperature and moisture. The annual cost of this effort exceeds \$500,000 in materials and labor. Despite this expense, the measured profiles are not as well suited to modeling as might be desired. Cost and slow ascent rate limit their temporal sampling interval (i.e., launch frequency) to 3 hours during Intensive Operation Periods (IOPs) and 6-8 hours during routine operations. In contrast, the radiation measurements used for comparison with model calculations have temporal resolutions and reporting intervals of a few minutes at most. Conversely, radiosondes have a much higher vertical spatial resolution, about 10 meters, than most models can use. Modelers generally reduce the vertical resolution of the soundings by averaging over the vertical layers of the model.

In an attempt to acquire profile measurements with temporal and spatial characteristics similar to the radiation measurements and more appropriate to models, ARM has deployed a variety of ground-based remote sensors. However, none of these remote sensors can provide a complete profile of tropospheric temperature or water vapor over the wide range of sky conditions and with the high reliability of the balloon-borne sounding system (BBSS). Consequently, the BBSS remains the primary profiling instrument.

Recently, Radiometrics Corporation developed a ground-based microwave radiometer capable of providing continuous, real-time vertical profiles of temperature, water vapor, and limited-resolution cloud liquid water from the surface to 10 km in nearly all weather conditions. The microwave radiometer profiler (MWRP), shown in Figure 1, offers a much finer temporal resolution and reporting interval (about 10 minutes) than the BBSS but a coarser vertical resolution that may be more appropriate for models.

To evaluate the performance of the new MWRP and the suitability of its profile measurements for driving typical radiation models, the radiometer was deployed at the

SGP central facility from 15 February to 8 August 2000. Since 15 September 2000, it has been deployed at the ARM North Slope of Alaska (NSA) central facility at Barrow, AK. Results of the evaluation to date are presented here.

The Microwave Radiometer Profiler

The microwave profiler is composed of two separate receivers in a single cabinet that share the same antenna and antenna-pointing system. A highly stable synthesizer permits tuning to a large number of frequencies within the receiver bandwidth. The temperature-profiling receiver measures the radiometric brightness temperature of the sky at seven frequencies corresponding to a complex of oxygen absorption lines between 51 and 59 GHz. The water-vapor-profiling receiver uses five frequencies extending from the center of the water vapor line at 22 GHz out to 30 GHz. Surface meteorological sensors measure air temperature, barometric pressure, and relative humidity. To improve the measurement of water vapor and cloud liquid water profiles, cloud base altitude information is obtained with an infrared thermometer. The calibration of the water-vapor-profiling receiver is maintained by continuous tipping curves. A liquid-nitrogen-cooled blackbody target is used to calibrate the temperature-profiling receiver. Detailed descriptions of the instrument and calibration procedures were given by Solheim et al. (1998a).

Profiles of temperature, water vapor, and cloud liquid water are obtained at 47 levels: from 0 to 1 km above ground level at 100-m intervals, and from 1 to 10 km at 250-m intervals. The profiles are derived from the measured brightness temperatures with neural network retrieval algorithms. For the SGP deployment, the neural network was trained with brightness temperatures calculated by using a microwave radiation transfer model for ten years of radiosonde profiles from Oklahoma City for February through August. For the NSA deployment, monthly retrievals were developed using ten years of radiosonde data for three month periods centered on the target month. The neural network retrieval and alternative retrieval methods were discussed by Solheim et al. (1998b).

Time-height color contours of temperature, water vapor density and liquid water content are presented in Figure 2 for January 13-17, 2001 at Barrow, Alaska. Except for the power outage, the data provide a continuous record of an interesting period of warming and moistening. Because this took place over a holiday weekend, no soundings are available for comparison. Typical profiles from the MWRP are compared with profiles from the BBSS in Figure 3 for inversion and lapse conditions at the SGP and NSA.

Statistical Comparisons

In Figure 4 we present statistical summaries of the comparison of MWRP profiles with soundings. We also compared the MWRP profiles from the SGP with profiles retrieved from the atmospherically emitted radiance interferometer (AERI) spectrometer, both alone (Smith, 1999) and when combined with profiles from the rapid update cycle (RUC) model. The latter are designated "AERI+." The AERI and AERI+ results are limited to clear-sky conditions. The SGP data were divided into two parts: the cooler, dryer period from mid-February to mid-May, and the warmer, moister period from mid-May to early August. The standard deviation about the ensemble mean of the BBSS profiles for each of these periods, often referred to as "climatology," is also plotted as a reference as are the mean BBSS profiles. The nearly all-weather capability of the MWRP allowed for about 35% more valid profiles coincident with BBSS soundings than were obtained with the AERI during the spring (193 vs. 145) and 20% more during the summer (150 vs. 124). Gueldner and Spaenkuch (2000) obtained similar results with an identical MWRP when they used a neural net retrieval; they also reported improved results with a regression-based retrieval.

Comparisons of precipitable water vapor (PWV) and liquid water path (LWP) from the MWRP with the 2-channel microwave radiometer (MWR) at the SGP are presented in Figure 5. The results show generally good agreement, but an increasing bias at high PWV, probably due to use of a single set of retrieval coefficients for the entire period rather than monthly retrievals as was done for the NSA. Comparison of LWP also shows good agreement, but reveals the need for higher resolution of the output format.

Conclusions

A new microwave radiometer profiler has been deployed at the ARM SGP and NSA facilities for extended periods for evaluation. The instrument has proved to be highly reliable and to perform well over a wide range of conditions. Comparisons with radiosondes demonstrate rms accuracy of 1-2 degrees Celsius for temperature at the SGP and NSA. For water vapor, an rms accuracy of 1-2 g/m³ or better was achieved at the SGP. Better than 0.5 g/m³ rms water vapor accuracy was achieved at the NSA, but the absolute amount of water vapor was quite small – only about 1 g/m³ near the ground on average – during the deployment period.

Future Work

Based on these results, Radiometrics is developing improved retrieval algorithms. In addition, Radiometrics is modifying the software to reduce the observing cycle time from 10 minutes to 2 minutes in order to reduce the variation in sky conditions during the measurement cycle, which can adversely affect the retrievals.

Acknowledgements

This work was supported by the Environmental Sciences Division, U. S. Department of Energy, Office of Science, Office of Biological and Environmental Research, under contract W-31-109-Eng-38, as part of the Atmospheric Radiation Measurement Program.

Wayne Feltz, University of Wisconsin, Space Science and Engineering Center provided the AERI+ retrievals.

References

- Gueldner, J. and D. Spaenkuch, 2000: Remote sensing of the thermodynamic state of the atmospheric boundary layer by microwave radiometry. *J. Atmos and Ocean. Tech.*, (in review).
- Smith, W. L., W. F. Feltz, R. O. Knuteson, H. R. Revercomb, H. B. Howell, and H. H. Wolf, 1999: The retrieval of planetary boundary layer structure using ground-based infrared spectral radiance measurements. *J. Atmos. Ocean. Tech.*, **16**, 323-333.
- Solheim, F. S., J. R. Godwin, and R. Ware, 1998a: Passive, ground-based remote sensing of temperature, water vapor, and cloud liquid profiles by a frequency-synthesized microwave radiometer. *Meteorologische Zeitschrift*, **7**, 370-376.
- Solheim, F. S., J. R. Godwin, E. R. Westwater, Y. Han, S. J. Keihm, K. Marsh, and R. Ware, 1998b: Radiometric profiling of temperature, water vapor, and cloud liquid water using various inversion methods. *Radio Sci.*, **33**, 393-404.

Figure Captions

Figure 1. The Microwave Radiometer Profiler (MWRP) deployed at the ARM NSA central facility in Barrow, Alaska. The infrared (10-micrometer wavelength) thermometer mounted on the MWRP provides an estimate of cloud base temperature, which is used to infer cloud base height and constrain the liquid water content retrieval.

Figure 2. MWRP profiles of temperature, water vapor, and cloud liquid from Barrow, Alaska for 13-17 January 2001 show a substantial warming and moistening above the surface temperature inversion.

Figure 3. MWRP profiles coincident with SGP soundings for 10 May 2000, 11:31 UTC (05:31 local) and 23:47 UTC (17:47 local), and the NSA sounding for 1 February 2001, 23:48 UTC. For the MWRP, relative humidity and dew point are calculated using the retrieved temperature and water vapor density profiles. The profiles labeled "RH max" indicates the ratio of the saturation mixing ratio over ice to the saturation mixing ratio over liquid water at the prevailing temperature; this is used as a quality check on the retrievals. These results illustrate typical performance for temperature inversion and lapse conditions.

Figure 4. The profiles of temperature and water vapor density derived from the MWRP brightness temperatures were compared with routine soundings and with profiles derived from the AERI spectrometer, both alone and in combination with the RUC model ("AERI+"). The mean difference ("bias") and the root-mean-square difference ("rms error") between the MWRP, AERI, or AERI+ profiles and the BBSS at the SGP are presented. Results of the comparison with soundings at Barrow, AK are also presented.

Figure 5. Comparisons of precipitable water vapor (PWV) and liquid water path (LWP) from the MWRP with the 2-channel microwave radiometer (MWR) at the SGP.



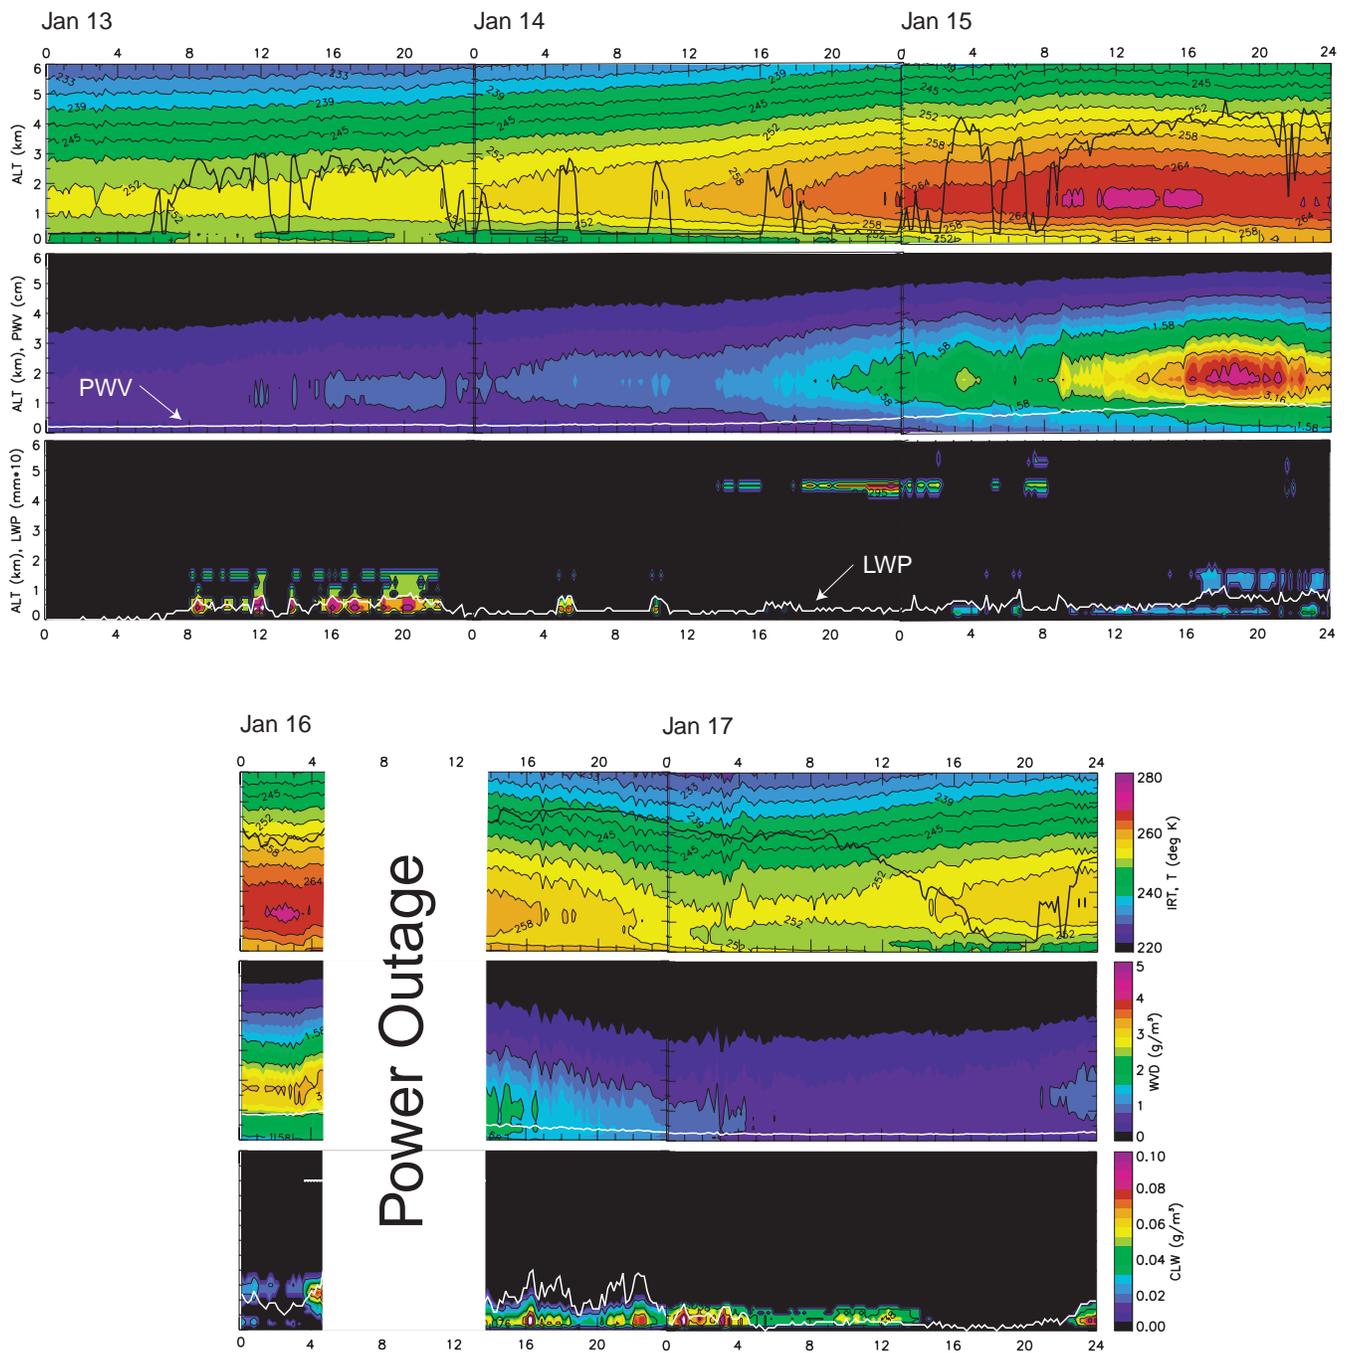
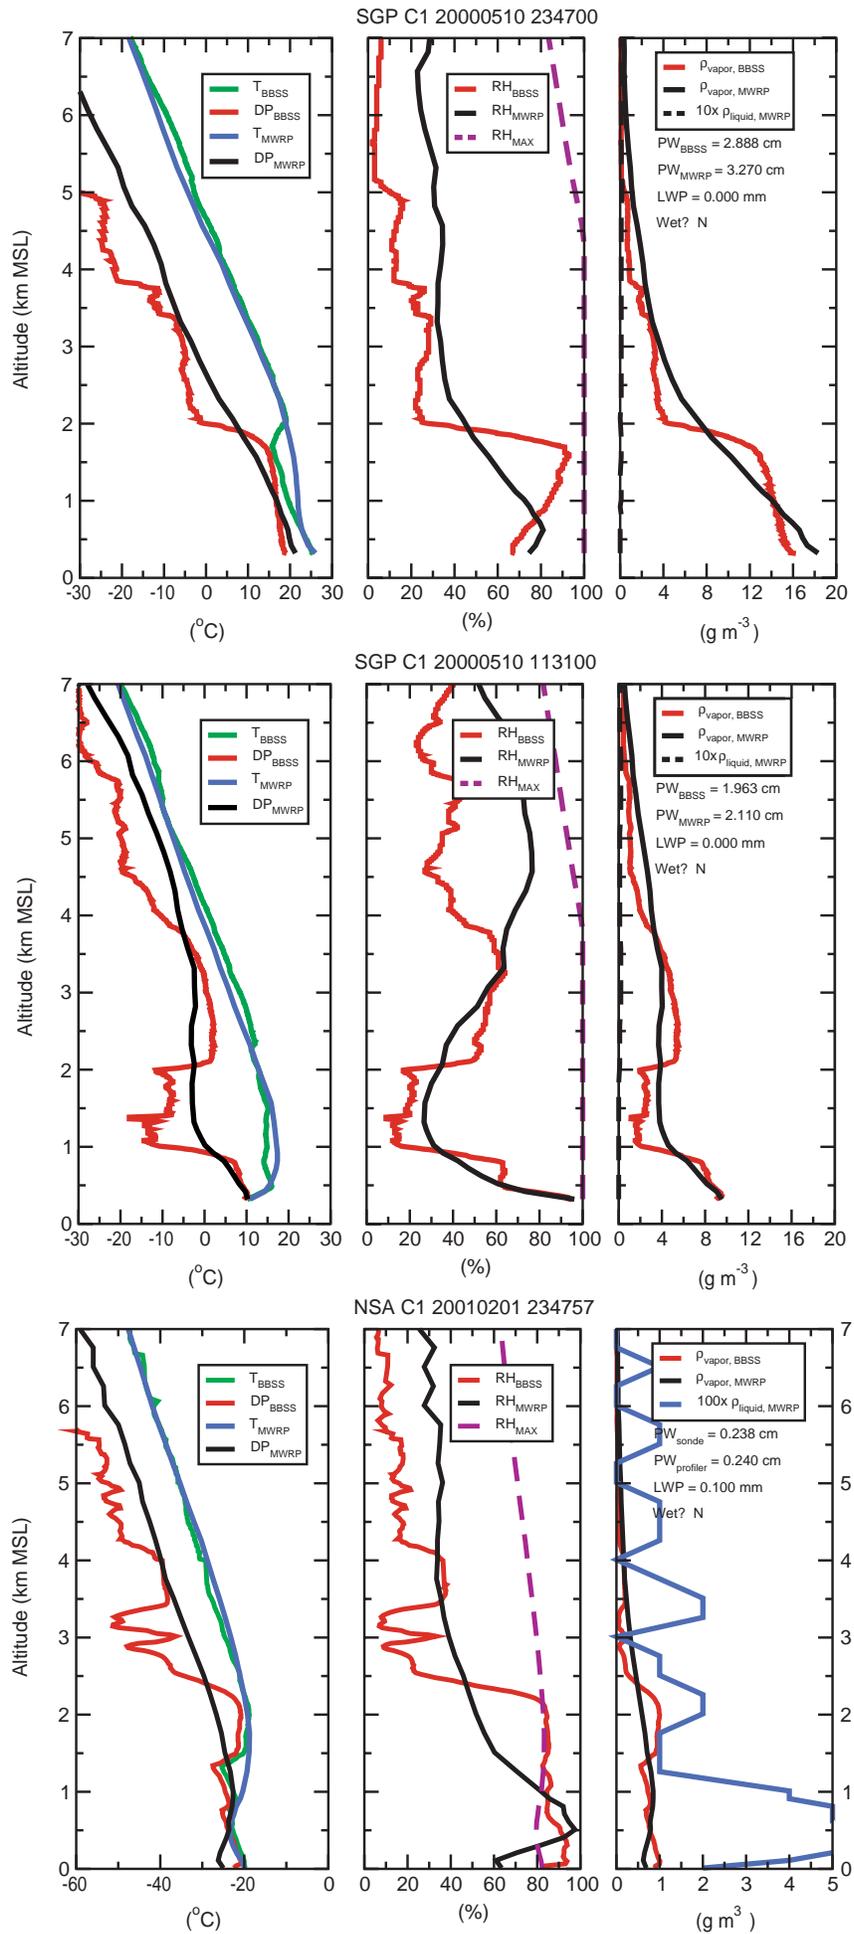


Figure 2

Figure 3



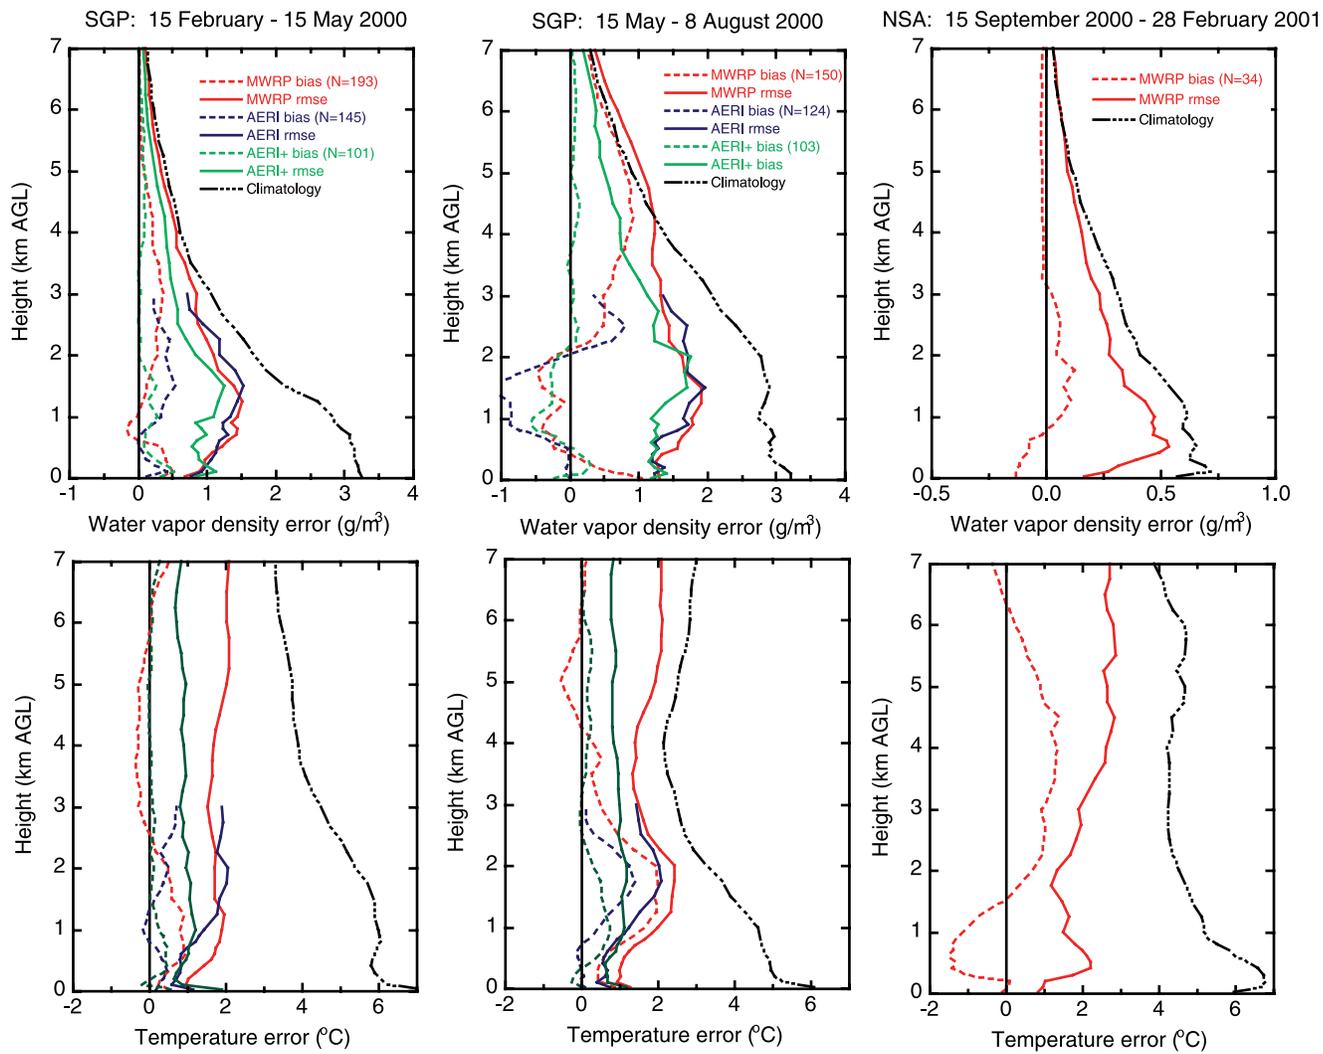


Figure 4

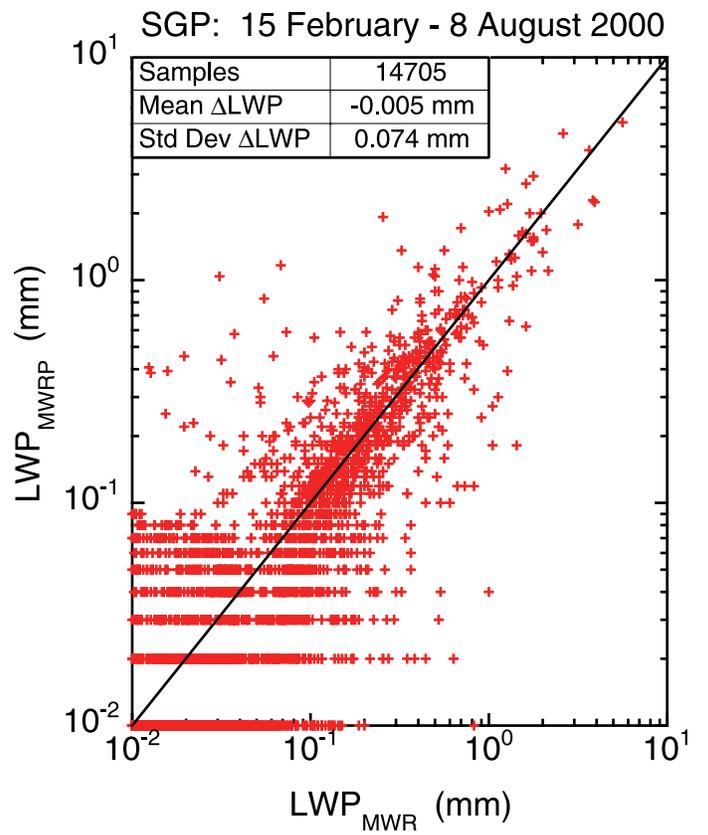
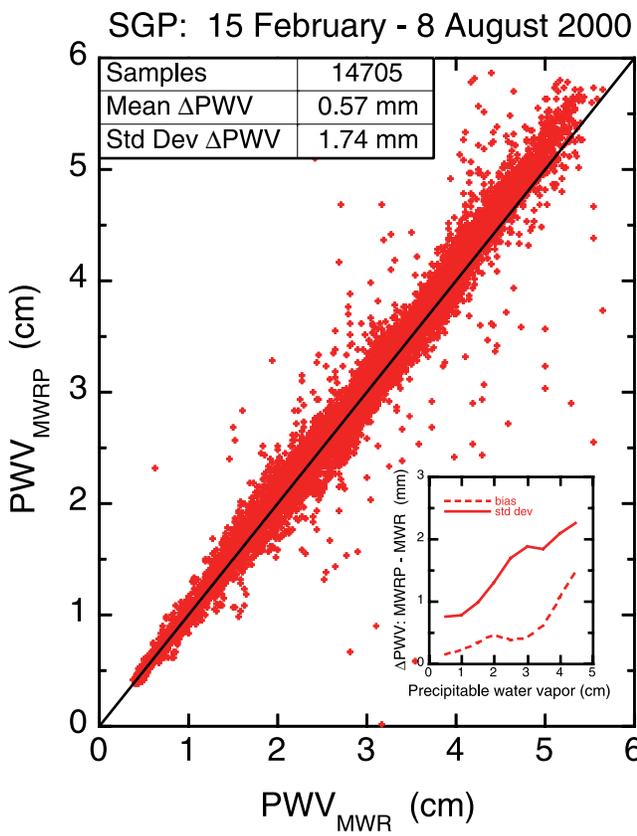


Figure 5